

Luminosity measurement by ZEUS @ HERA-II

W. Schmidke
MPI, Munich

EIC meeting
Stony Brook 12.01.10


Outline

- The process: $ep \rightarrow ep\gamma$ & measurement requirements
- ZEUS LUMI system components & layout
- Photon calorimeter: 'classic' direct γ measurement
- LUMI pair spectrometer: novel features
- Results
- Lessons

Process: BH $ep \rightarrow e\gamma$

ep bremsstrahlung (Bethe, Heitler 1934)


- High rate, σ_{BH} known to $<0.5\%$
- Steeply falling w/ E_γ (IR divergent)
- Drops to zero @ endpoint $E_\gamma = E_e$
- Sharply forward-peaked @ HERA θ_γ dominated by e-beam p_T spread

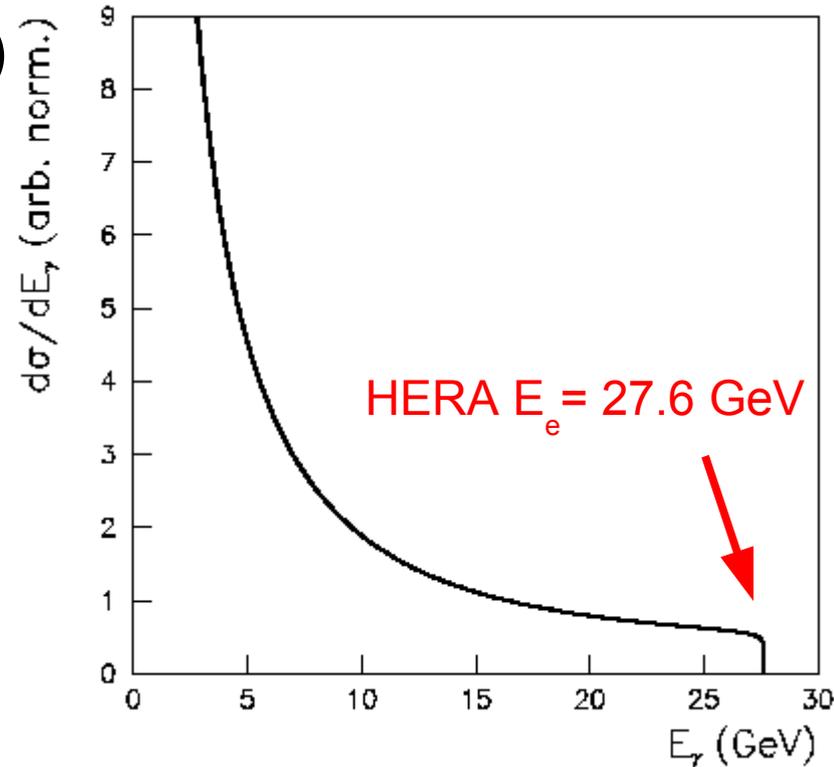

Photon measurement requirements


- E_γ in range few GeV \rightarrow ~ 25 GeV
- @ high L_{inst} , low $E_\gamma > 1$ γ per HERA bunch
- Measure θ_γ , correct for aperture loss

aperture as measured by foil exposed to sync. rad.

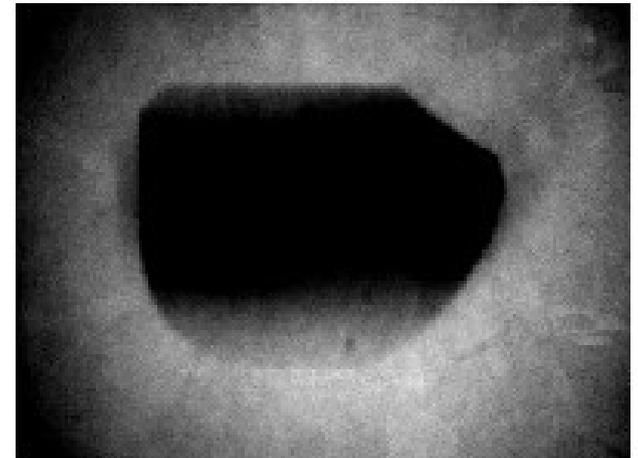

ZEUS LUMI system: 2 γ detectors

~100 m from I.P.

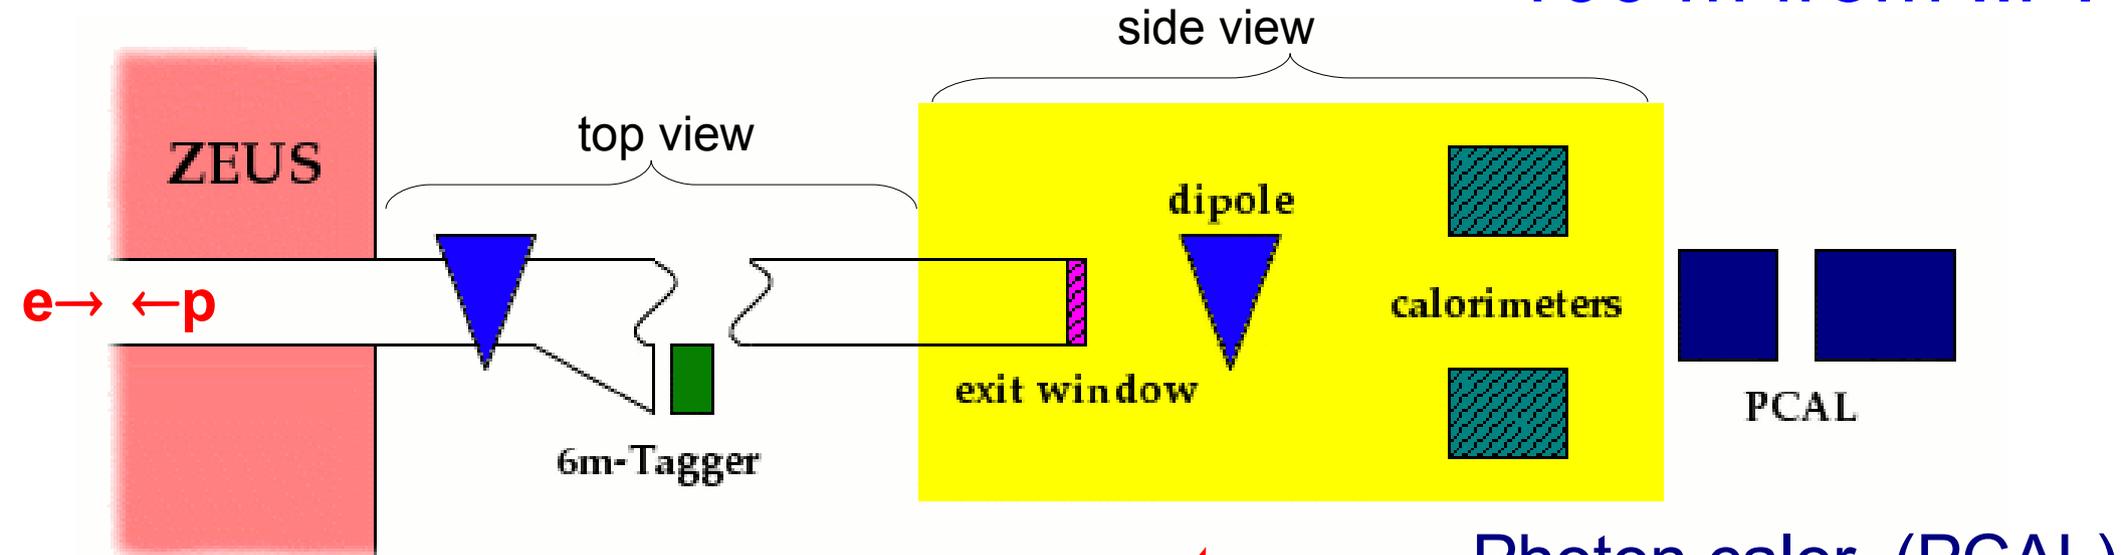

e tagger @ 6m from I.P.

- Measure scattered e
- W -scint. spaghetti calor.
- Check photon accept. (work in progress...)
- Also for physics: tag high W photoprod.
- Not discussed more here...


Photon calor. (PCAL)

- Direct measure γ

Pair spectrometer

- Measure pairs from $\gamma \rightarrow e^+e^-$ in exit window

PCAL: direct γ measurement

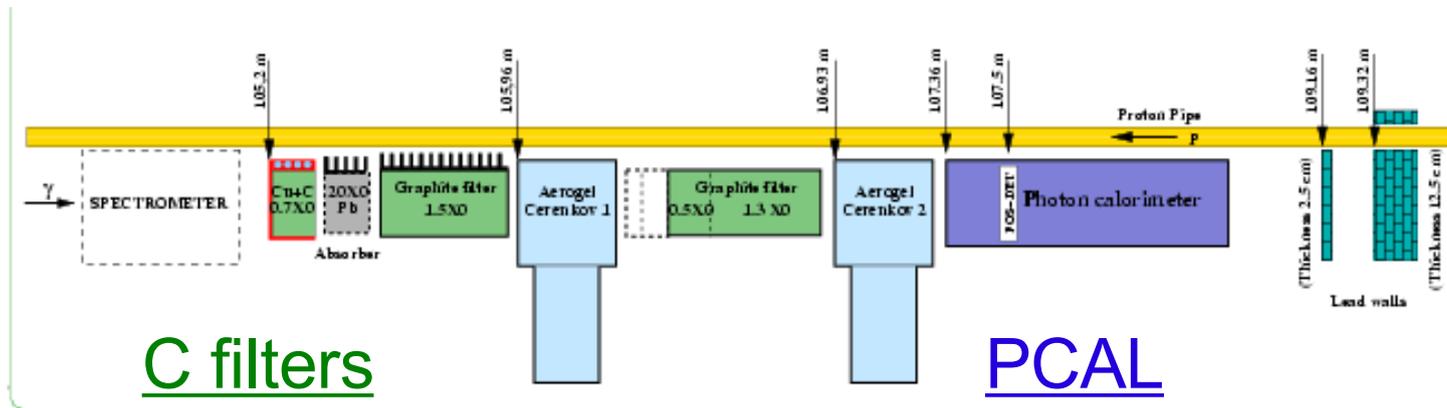

C filters

- $\sim 3-4 X_0$
- w/ Aerogel Ckv. det.
(not used for LUMI,
used for physics)

PCAL

- Pb-scint. sandwich
- Scint. hodoscope
for position recon.

- PCAL sits in direct γ beam, also **primary syc. rad.** fan
- PCAL *must* be shielded: C/graphite filters
- Serious resolution degradation; must be MC modeled
- Does provide soft cutoff $E_\gamma < \text{few hundred MeV}$,
protect against IR divergence in B-H spectrum




PCAL

Calibration: endpoint B-H spectrum

- Colliding ep bunch endpoint smeared
- Use unpaired e -only HERA bunches
 - e -gas rate $\sim 10^{-2}$ ep rate
 - e -gas spectrum \sim B-H undistorted
 - MC fit to endpoint

LUMI measurement

- Scalers count γ 's $E_\gamma >$ threshold
- Spectrum distorted by
 - multiple γ 's / bunch \times ing (pileup)
- Use several thresholds, compare to MC for various n_γ
 - e.g.: $E_\gamma > 0.1$ GeV, $n_\gamma = 0, 0.5, 1, 1.9$
- Several % correction:
 - requires precise PCAL MC model

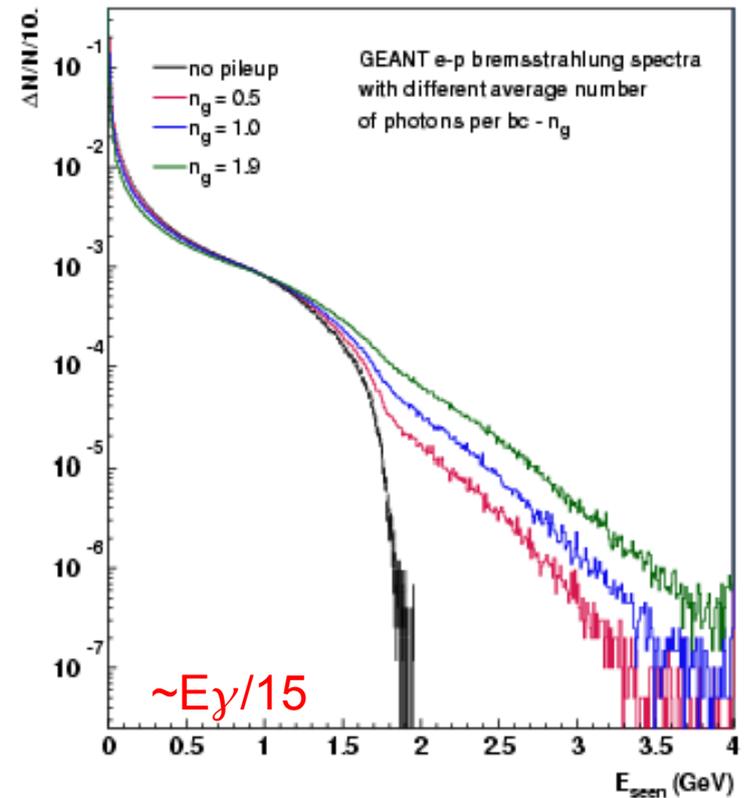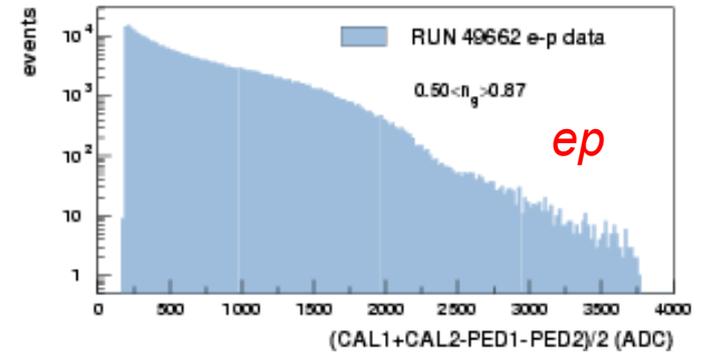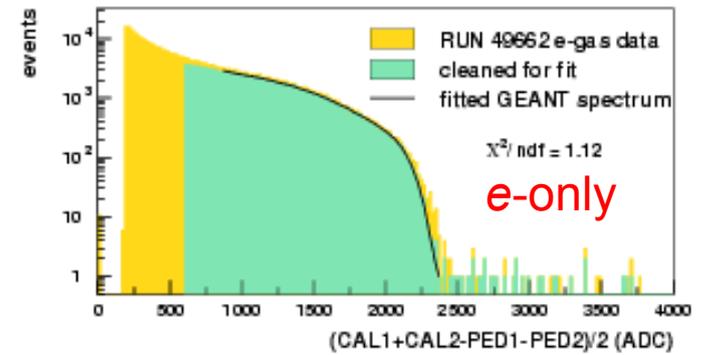


PCAL

Beam-size effect

- Impact parameter limited by transverse beam size: low E_γ suppressed
- Observed e.g. VEPP e^+e^- , HERA-I ep
- HERA-II smaller beam size, stronger effect $>2\%$

Other effects, corrections:


- Electronics pileup (pulse overlaps)
- Pedestal shift from sync. rad.

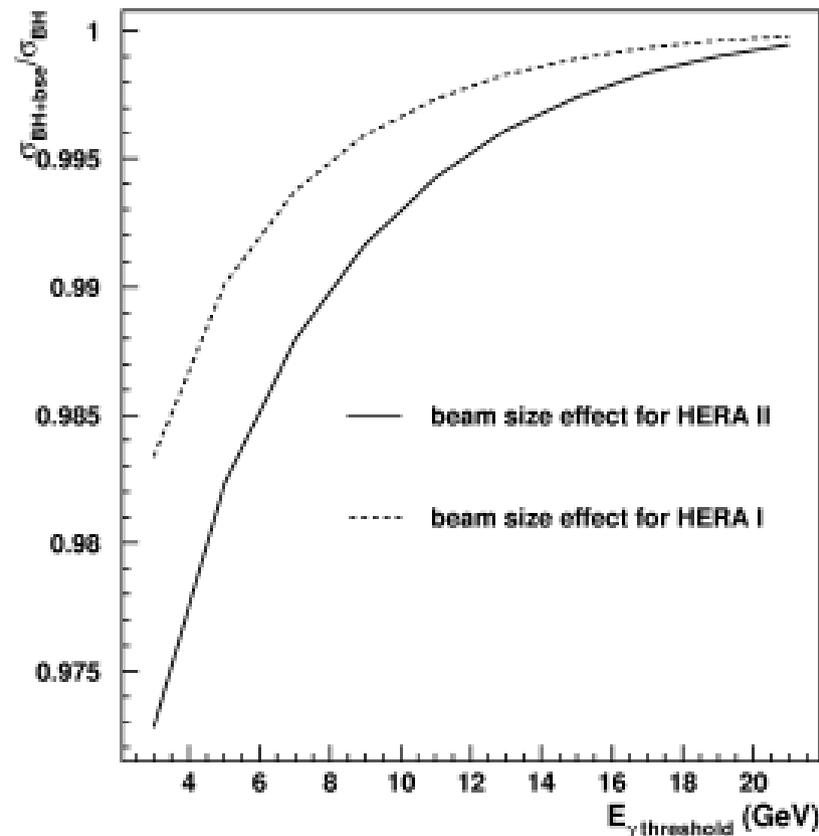

PCAL summary:

- Concept & detector simple
- Complications: shielding, high rates, low E_γ
- Large (several %) corrections require accurate MC modeling

Pair Spectrometer

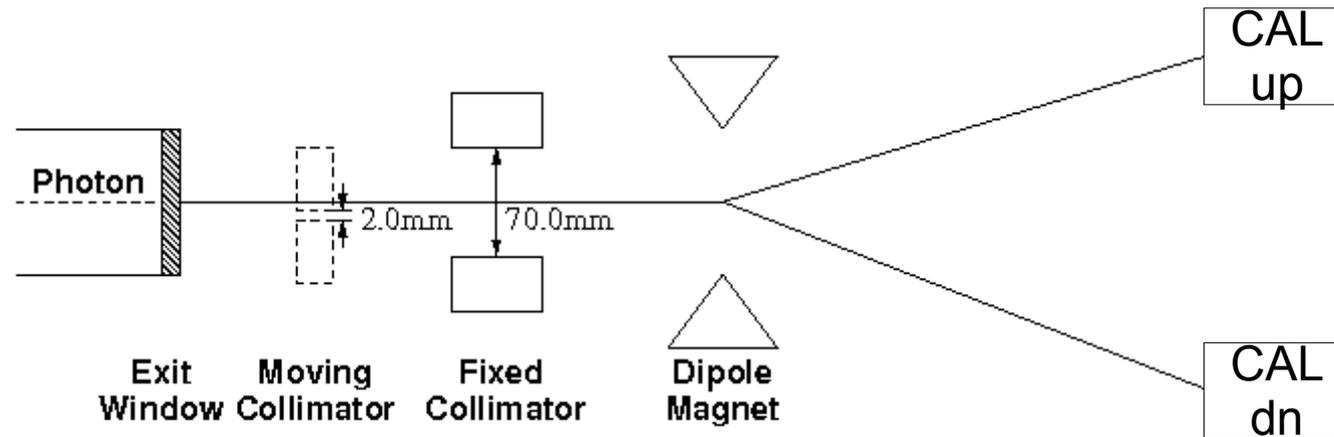

- In exit window $\sim 9\%$ $\gamma \rightarrow e^+e^-$ conversions \Rightarrow **>10 rate reduction**
- Pair separated vertically by dipole $\int Bdl \approx 0.3 \text{ T}\cdot\text{m} \approx 0.1 \text{ GeV } p_T$
- e^+, e^- detected in W-scint. sandwich calorimeters

horiz., vert. segmented for position **recon.** \Rightarrow **out of primary sync. rad. fan**

Calibration:

- Insert 'moving collimator', defines narrow vert. pair position
- Now a 'true spectrometer':

From $\int Bdl$, distance to calorimeters,



vertical position in calorimeter determines energies e^+, e^-

Spectrometer: calibration

- Check endpoint of B-H spectrum (special run w/ higher dipole field):
- E-scale agrees $\sim 1\%$




However:

- Calorimeters were not well shielded from secondary synchrotron radiation
- Gains varied considerably; here worst channel last ~ 3 years HERA operation:
- Gain dropped in HERA operation; recovered HERA shutdowns (it was wavelength shifters)
- A calorimetry based E_γ LUMI measurement problematic
- Solution in a few slides...

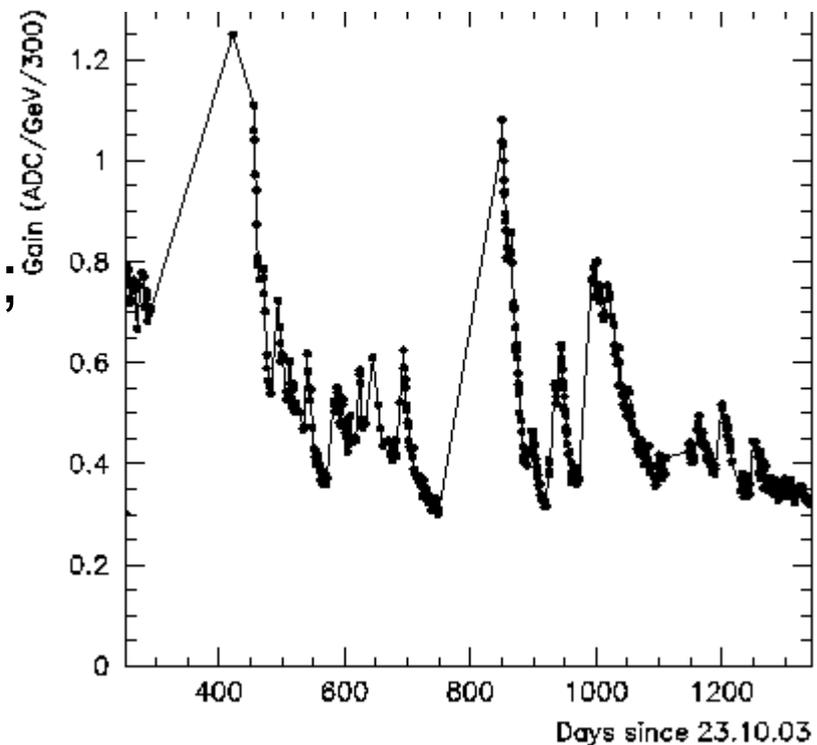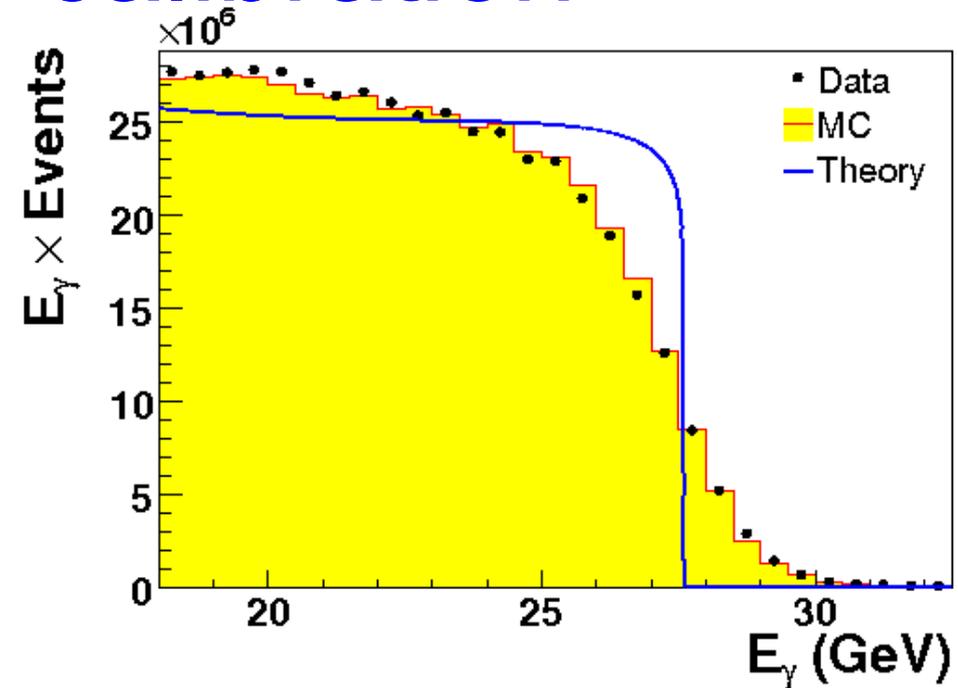



Spectrometer: LUMI measurement

- Count up, down calor. coincidences for ~ 16 sec. (ZEUS int. time)
- Accumulate E_{γ} , X_{γ} , Y_{γ} histograms
- Account for ellipse tilt:
- Fit MC for photon beam (X_0 , Y_0)
and gaussian spread major-/minor axes
 \Rightarrow accept. corr. for aperture, spec. geom.
- Fits made to X_{γ} , Y_{γ} distributions, good:

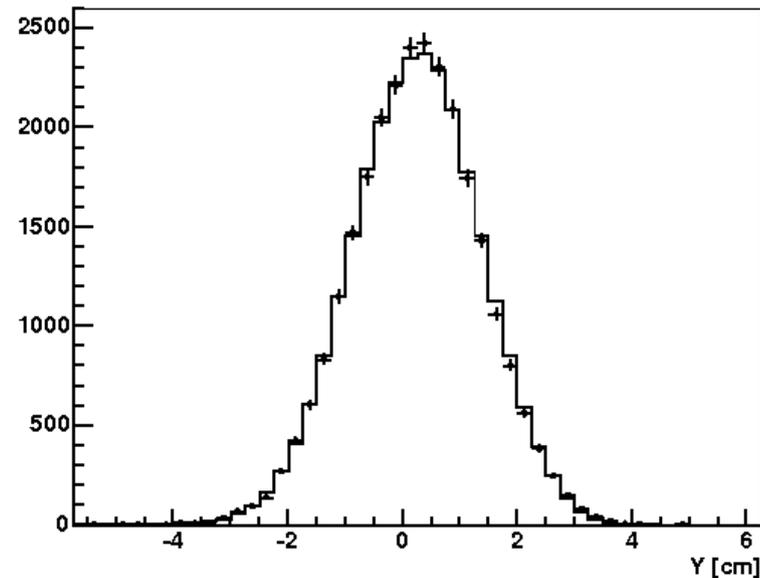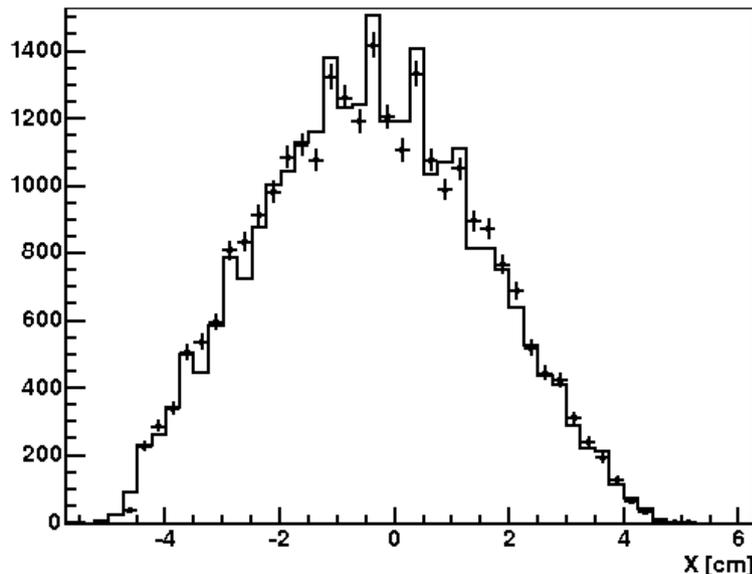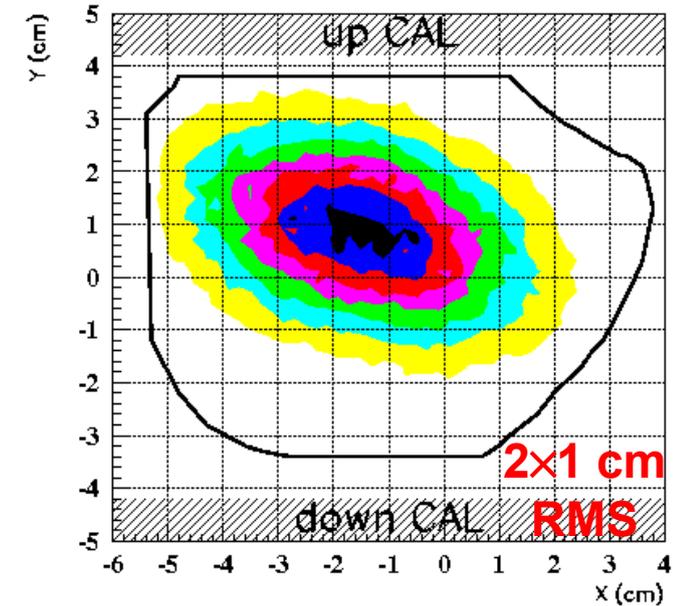

Spectrometer: LUMI measurement

- Fit not made to E_γ spectrum, but resulting MC prediction agrees well:
- Can also reconstruct $\int B dl$ each event
- Compare difference from nominal $\int B dl$ to MC prediction:
- Tail @ low $\Delta \int B dl$ due to $\gamma \rightarrow e^+ e^-$ in *air inside dipole gap*
- Good agreement data \leftrightarrow MC

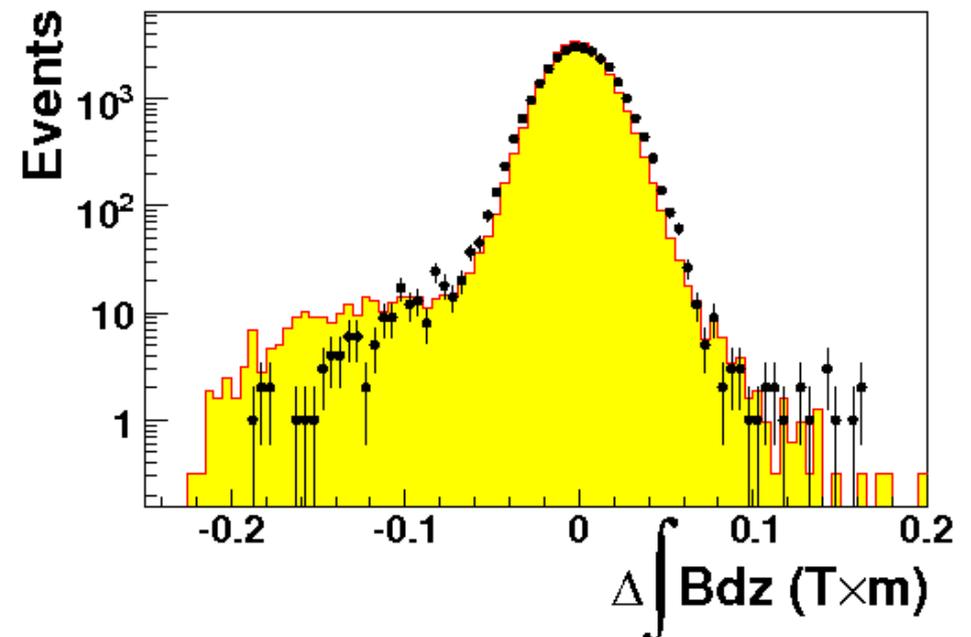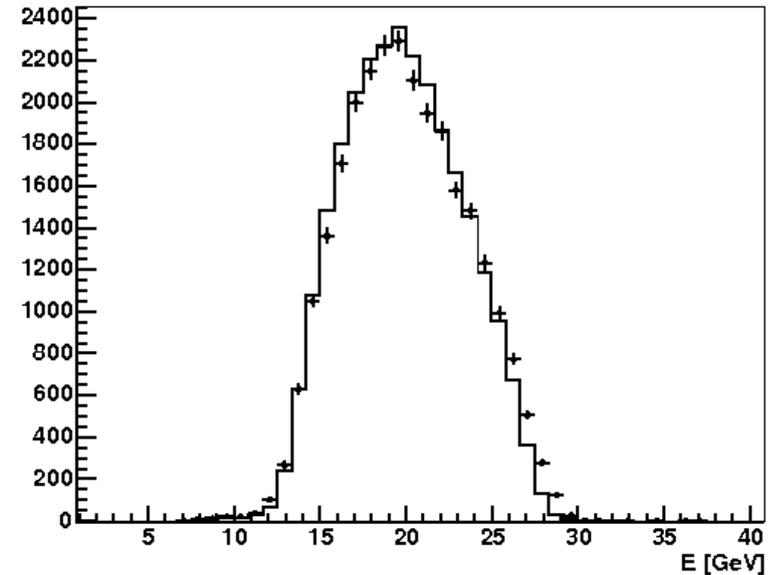


MC verified by independent checks, accurate acceptance


Spectrometer: E_γ range

- Consider pair midway between calorimeters, with equal shared energy e^+, e^-

- There is a minimum E_γ which will produce a coincidence; lower E_γ either e^+ or e^- will miss outside calorimeters:

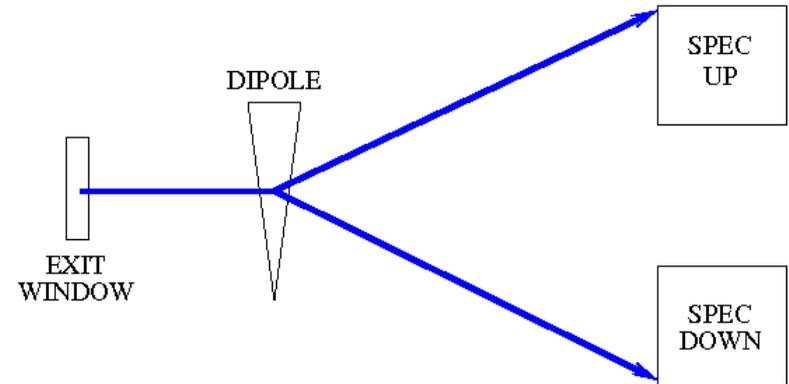


- Similarly there is a maximum E_γ which will produce a coincidence; higher E_γ either e^+ or e^- will miss inside calorimeters:

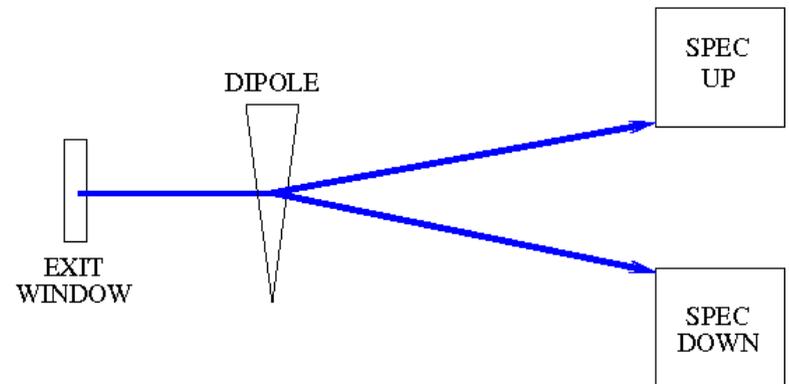

Spectrometer: E_γ range


- Define the energy sharing $z = E_{e^+}/E_\gamma$, $0 \leq z \leq 1$
- Then can plot SPEC acceptance in the (E_γ, z) plane, inside kite-shaped region:
- Insets show the pair configurations at edges, corners of acceptance

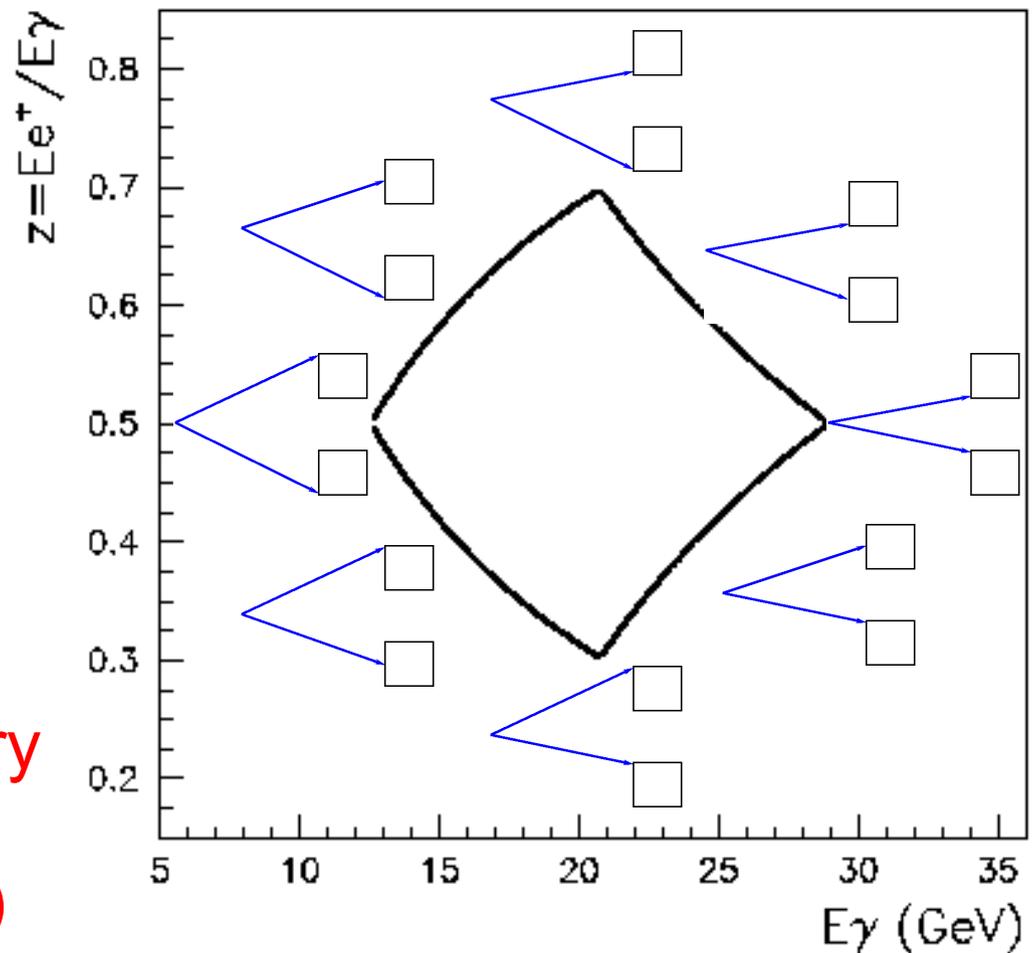

- Pair spectrometer geometry defines an inherent region of acceptance in the (E_γ, z)


Spectrometer: E_γ range

- The energy sharing distribution symmetric, slightly peaked @ $z=0,1$:
- Integrate over acceptance region to get acceptance vs. E_γ
- Simple calculation describes features of full MC simulation including beam spread, resolutions, ...

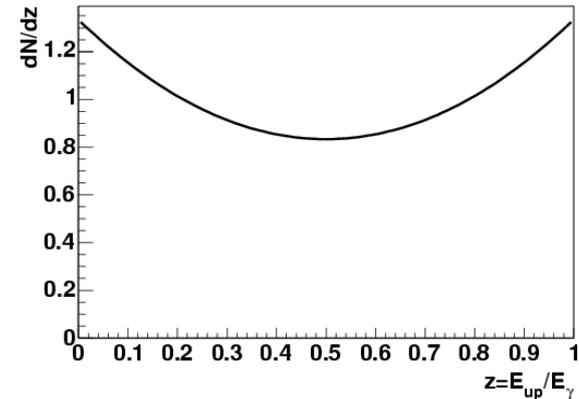


Pair spectrometer geometry defines an inherent E_γ range:

- Low E_γ cutoff, protect against IR divergence of B-H spectrum, low E_γ beam-size effects
- Fiducial regions of detectors weakly dependent on calibration, protect against gain variations

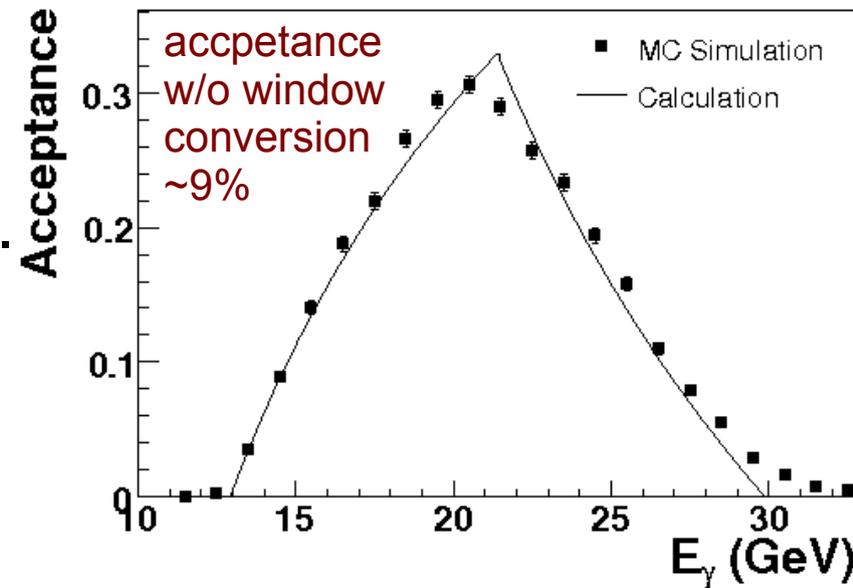

Spectrometer: pileup


- Can have >1 γ conversion in 1 HERA bunch \times ing
- 2 pairs that would not each make a coincidence could make one:

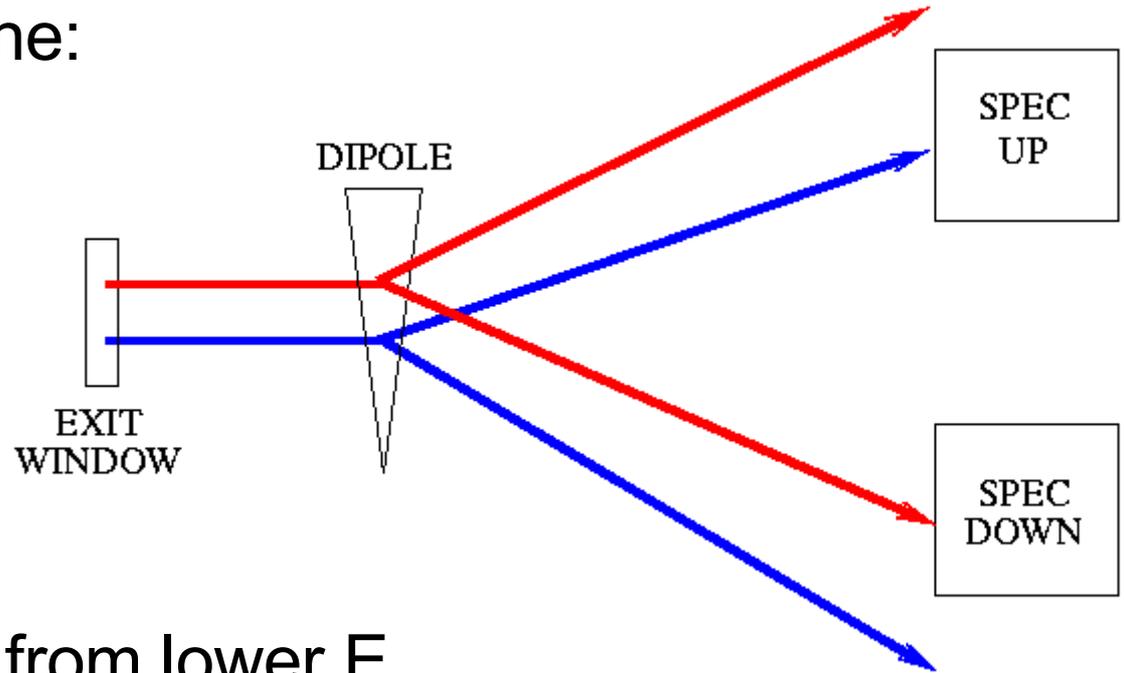

- Such single hits can come from lower E_{γ} than possible for true coincidences \Rightarrow potentially high rate
- This leads to *overcounting* of coincidences at high L_{inst}

Spectrometer: pileup


- The spectrometer DAQ did baseline (pedestal) subtraction by subtracting channel energies from previous HERA bunch
- A single from a previous bunch conversion (---) could overlap a valid coincidence, stealing its energy and failing threshold cuts

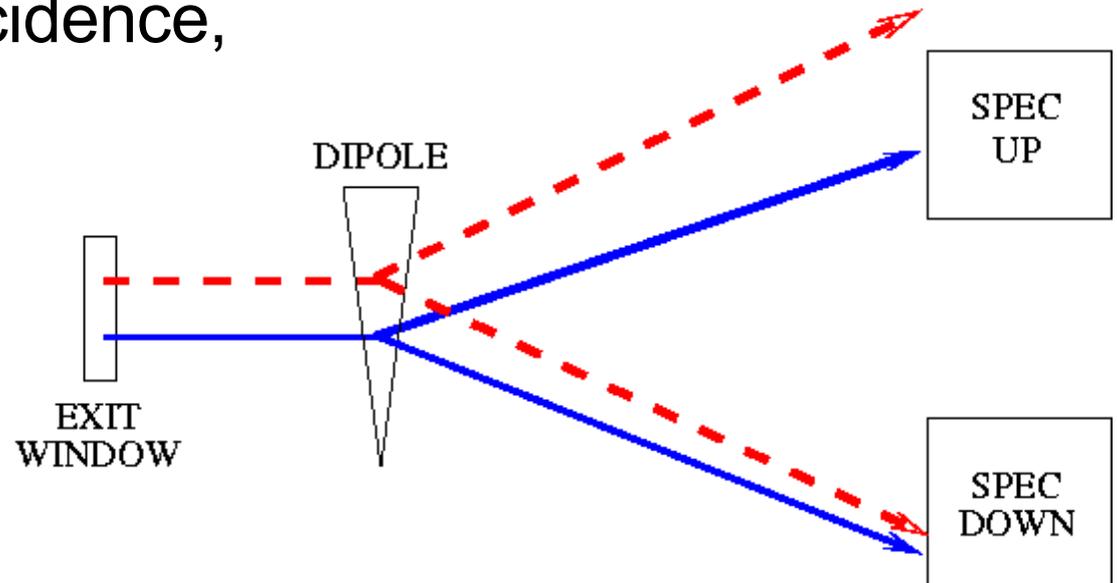

- Such single hits can come from lower E_γ than possible for true coincidences \Rightarrow potentially high rate
- This leads to *undercounting* of coincidences at high L_{inst}

Spectrometer: pileup

- Model in MC: overlap conversions, add/subtract channel energies:
- As expected 2 effects opposite sign, **and nearly cancel**
- Total pileup correction $< 0.5\%$ @ highest HERA L_{inst}

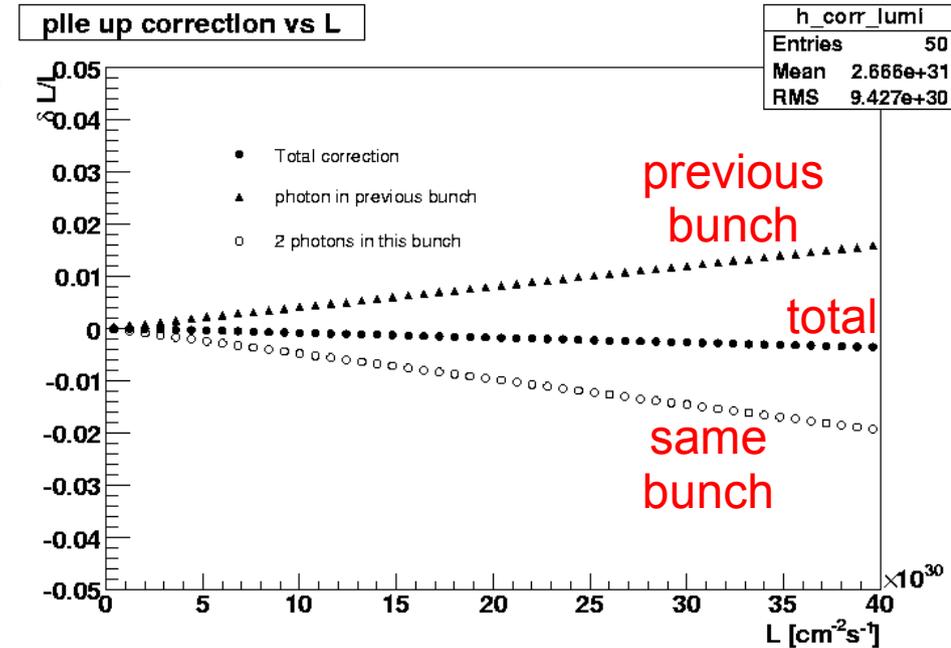


Spectrometer: summary

- Concept & detector more complex than PCAL, but:
- Straightforward calibration, E-scale $\sim 1\%$
- Natural E_γ range: no low E_γ complications, weak dependence on calorimeter calibration
- Negligible pileup correction

Results

PCAL & SPEC comparison:

- PCAL & SPEC operated and analyzed by two independent groups
- They agree within 1%
- Plotted here L weighted ratio per physics run:

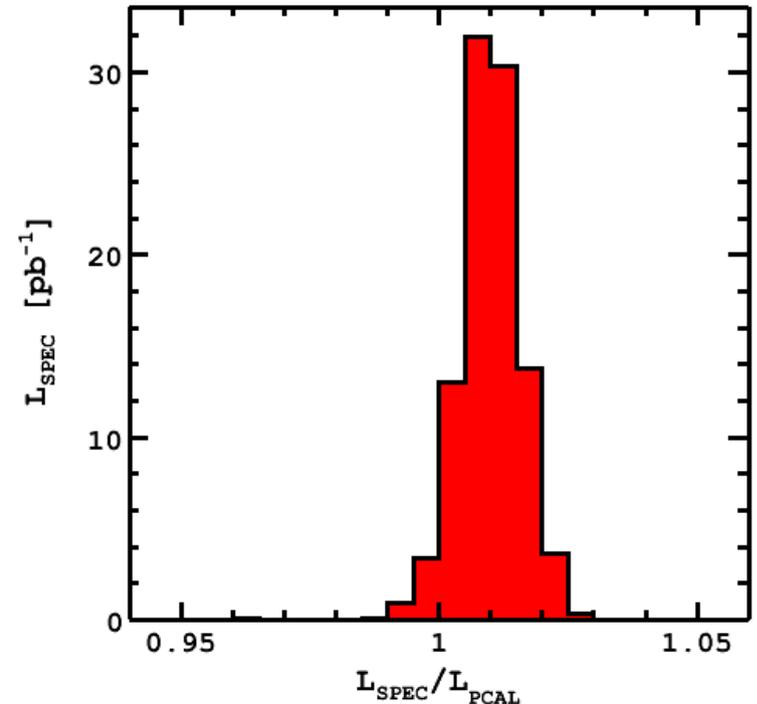

Systematic uncertainties:

- Both PCAL & SPEC have sys. uncert. **$\pm 2.5\%$**
- PCAL uncert. comes equally from the several corrections, probably irreducible
- SPEC uncert. dominated by window conversion prob.: **$\pm 2\%$** already improvement found; window being remeasured...
- Hope to improve further with e-tagger studies...

Lessons

PCAL & SPEC both useful for future installation:

- Complement each other well:
 - PCAL simple concept, detector; tricky LUMI analysis
 - SPEC complex idea hardware; novel features aid LUMI meas.
- Also: backup, redundancy, cross checks...
 - SPEC (recycled hardware, HV) failed several periods
- PCAL also useful for initial state radiation tagging
- SPEC has several parameters that can be tuned:
 - window thickness (conversion probability)
 - dipole field
 - detector geometry, fiducial volume


Not discussed in detail here, but
electron tagging very useful:

- Measure LUMI acceptances, other checks...
- Low angle e tagging already EIC priority

EXTRAS

HERA tilt scans

- HERA made extreme tilts of e beam to probe aperture edges:

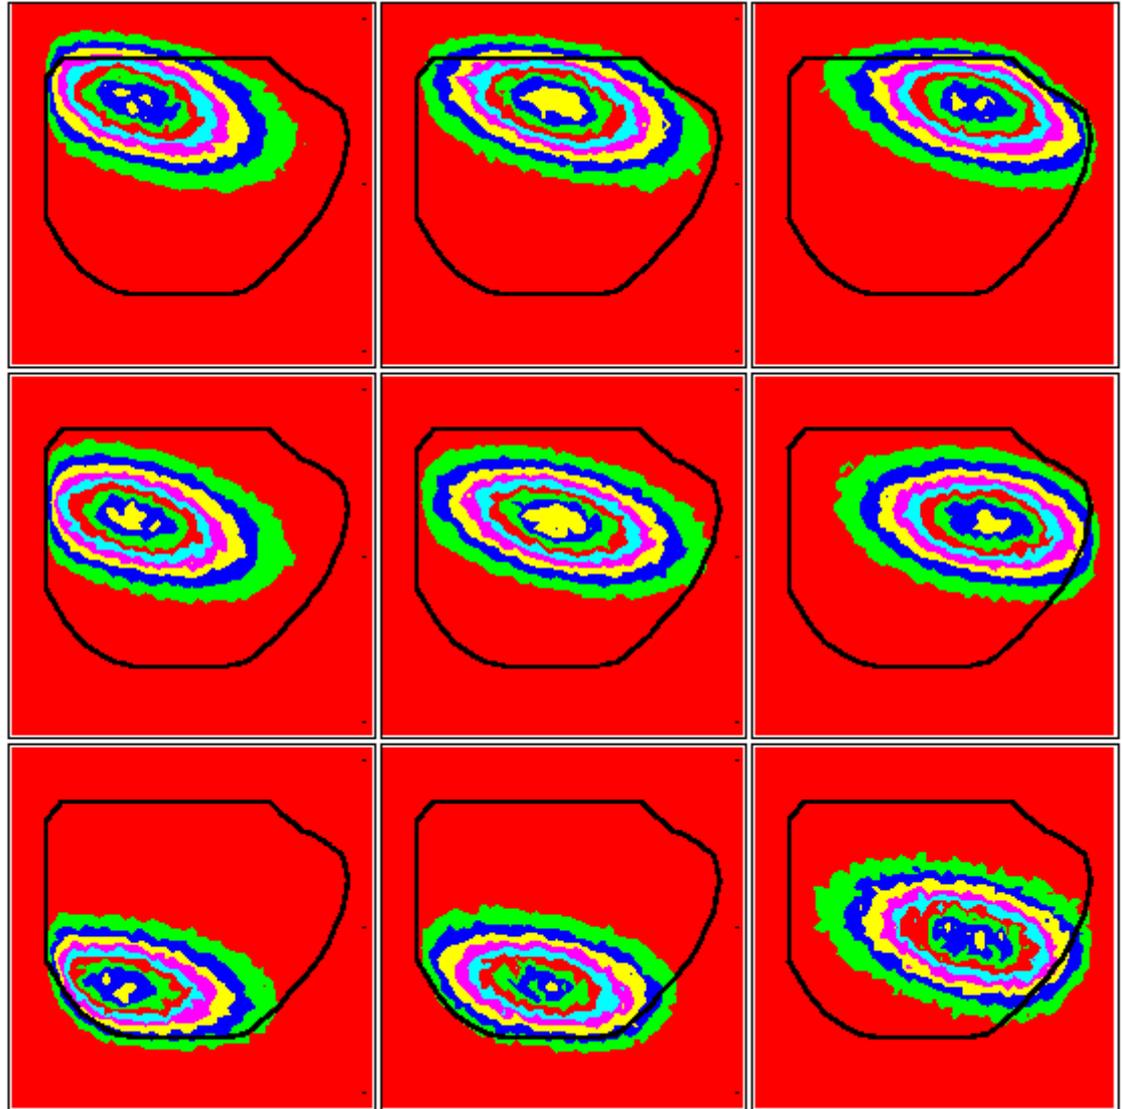

(E_γ, z) plane acceptance

- Acceptance region in (E_γ, z) plane varies with γ vertical position
- Shown here for 0, 1, 2 cm above SPEC midpoint

